

Angular Rate Sensor

Owner's Manual

PART NUMBER: ARS-G152



WATSON INDUSTRIES, INC.
3035 MELBY STREET
EAU CLAIRE, WI 54703

Phone: (715) 839-0628

Fax: (715) 839-8248

Email: support@watson-gyro.com

Table of Contents

Introduction.....	3
Product Description	3
Installation	3
Orientation	3
Mounting.....	3
Environment:	3
Power	3
Calibration	4
Operation	4
Initialization	4
Interface	4
RS-232 Output Format.....	4
RS-232 Input Commands.....	5
Analog Outputs	7
Built in Test Digital Output	7
Specifications.....	8
Connections	9
Dimensions	9
WARNING	10
DISCLAIMER	10
WARRANTY.....	10
PRODUCT LIFE	10
Appendix B.....	14
Activating Command Mode (Double Spacebar Mode).....	14
Accessing the Main Menu.....	14
Appendix B.1 Set Output Channels	14
Appendix B.2 List Output Channels	15
Appendix B.3 Set Analog Voltage Range.....	15
Appendix B.4 Set Output Bandwidth.....	16
Appendix B.5 Set Binary Output Format.....	16
Appendix B.6 Set Baud Rate	17
Appendix C Binary Output Format	18
Appendix C.1 Two Byte Binary Data Format.....	18
Appendix C.2 Three Byte Binary Data Format.....	20

Watson Industries prides itself on solving customer problems and serving their needs in a timely fashion. This manual is intended to facilitate this goal and to provide written information about your product. We ask that you carefully read this manual. Becoming familiar with the manual will help you understand the product’s capabilities and limitations, as well as provide you with a basic understanding of its operation. If, after reading the manual, you require further assistance, do not hesitate to call Watson Industries with your questions and comments.

CAUTION!

Watson Sensors are rugged devices that have been used successfully in a number of harsh environments. The components have been qualified to withstand a mechanical shock of 500g 's or greater, and most enclosures provide near that level of protection. However, dropping a sensor from waist height onto a hard floor can cause a shock level of 600g's. At this level, given some resonance, damage is possible.

Introduction

The Watson Industries Angular Rate Gyro represents a significant advancement in inertial sensor technology. It is a highly accurate and rugged device with many advantages over other types of angular rate devices. This manual describes operation of the Watson Industries ARS and also provides useful application information to the system designer.

Product Description

The Watson Industries angular rate gyro is a solid state, single axis angular rate sensor. The gyro provides a voltage proportional to the rate of turn about its sensitive axis. During rotation, positive voltage output occurs in the direction of the rotational arrow indicated in figure 2. There are four analog outputs available (400°/s , 200°/s , 100°/s , 50°/s fullscale). The analog outputs are user selectable between unipolar (0-5 VDC) or bipolar (± 5 VDC). The bandwidth is also user adjustable from 5 to 200 Hz. A power supply, providing +8 to +45 Volts DC, is required to operate the unit.

Installation

Orientation

The base of the unit is to be mounted on top of a horizontal surface. The gyro drawing, with pinout, is located in figure 2. The gyro is a rugged device and will withstand harsh environments. However, due attention needs to be paid to the nature of the sensor and its prime function, which is to measure angular rate.

Mounting

The unit has three 0.12" diameter mounting holes for using three # 4 (or 3 mm) screws. To avoid distortion, the unit must be attached to a clean, flat surface, and the fasteners must be tightened evenly.

Environment:

Avoid mounting sites that are subject to significant temperature variation over the duration of the test. Temperature variation will induce significant rate sensor bias drift, which will reflect in poor angular rate accuracy.

For all applications, it is preferable to install the device where linear dynamic effects are minimized.

Power

This unit has an internal regulator to allow operation over a wide voltage input range. Best operation is obtained at either +12 or +24 VDC level, although operation is fully satisfactory down to +8 VDC and up to +45 VDC. The power ground is already connected internally to the signal ground. Do not connect the ground wires externally. Power consumption of the unit is about 0.7W. Internal capacitors are provided to remove a reasonable level of power line noise, however, capacitors should be added for long power line wiring or if noise is induced from other loads on the circuit.

Calibration

The ARS is calibrated at the factory before it is shipped to the user. It is recommended that the unit be examined, preferably at the factory annually for evaluation and recalibration.

Operation

Initialization

The initialization time typically takes 4 to 5 seconds. During this time, a message is sent from the unit via the RS-232 serial link. This message gives information about the Gyro such as the full model number, serial number, and firmware revision. The message can be read by using a terminal program or by using the terminal mode of Watson Industries' communication software.


Interface

RS-232 Output Format

The standard RS-232 output is received from the 12-pin connector. The digital output pin map can be found in the Connections section of this manual. The RS-232 output consists of a string of decimal ASCII characters sent asynchronously at regular intervals. By default, the string is sent at 9600 baud with eight data bits, one stop bit and no parity. The RS-232 signal is referenced to signal ground. The number of strings sent per second depends on the baud rate and the output format. The maximum rate is 250 strings per second. The contents of a typical string are formed as follows: (See Appendix B for information on how to change the data string.)

1. A single letter and a space used to indicate the start of the data string. The letter "I" indicates the start of an inertial data string.
2. A eight character string representing the angular rate starting with a space, then a "+" or a "-", followed by three digits, a decimal point and two digits for up to ± 399.99 °/second.
3. The string is terminated by a carriage return. There will then be a short interval with no data transmission before the next string begins.

Example:

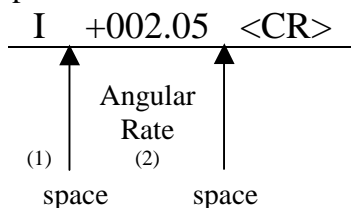

The data items transmitted can be changed by using the menu system (see Appendix B). More channels are available for output (see Appendix A).

The system is protected from inadvertent write-over of the EEPROM by requiring two spacebar commands during the initialization interval to access the EEPROM or related functions.

The baud rate may be changed from the nominal value of 9600 baud by modifying the default value in the EEPROM of the unit to 38.4K, 19.2K, or 4800 baud.

A text header that is sent by the Gyro during initialization identifies the unit by part number and by serial number and gives the date of last calibration. Additionally, a line of text characters that identifies the data channel columns is sent if the serial output is set to ASCII decimal. This whole message can be temporarily (or as a default) suppressed or restored by a "*" command from the interfacing computer.

Data transmission sent by the ADS can also be suppressed or restored by a "+" command from the interfacing computer. This command is typically used when only analog data is used as a noise reduction measure.

The other output format available is a binary format. The binary format provides generally the same information as the decimal ASCII format, but in a compact binary file message. In this format, there are nominally 3 bytes sent that represent 1 twenty-one bit gyro output followed by a carriage return. This format is for highly experienced users only. See Appendix C for more information. Consult the factory for further details.

RS-232 Input Commands

The RS-232 input commands are provided for the purpose of unit test and installation set-up. Use the same parameters that are used for the output (9600 baud ASCII nominal, or as reset in the units EEPROM).

Note: Many commands require command or "Double spacebar mode" in order to access them. For more information on how to activate Command Mode, see the instructions in Appendix B.

These commands are available to the user (others are used at the factory for alignment and calibration):

1. An "!" will reinitialize the unit. Further, access to initialization is inhibited such that a spacebar command must be sent within about 2 seconds of the "!" command for initialization to be engaged. Command mode is not required to access this function.
2. A "Z" or "z" will reset the timer channel counter. The timer channel counts seconds since the last reset. This command sets the timer back to zero. Command mode is not required to access this function.
3. A "L" or "l" will transmit a line of labels corresponding to the data channels that are currently selected for output. See Appendix A for information about the data channels and their labels. Command mode is required for access to this command.
4. An "_" command will change the output format to decimal ASCII. This change is made non-volatile in the unit on EEPROM by keying in the quote (") character. Command mode is required for access to this command.
5. A "^" command will change the output format to binary. This change is made non-volatile in the unit on EEPROM by keying in the quote (") character. Command mode is required for access to this command.
6. A ":" command will toggle the output to send a frame of data upon receiving any non-command character (On to Off; Off to On). This change is made non-volatile in the unit on

EEPROM by keying in the quote (“) character. Command mode is required for access to this command.

Note: To test if this command is active when the unit is not flowing data, send a carriage return (or any other non-command character to the sensor, and observe if there is any output.

7. A “+” command will suppress or restore the transmission of data. This command will toggle the data transmission (On to Off; Off to On). Command mode is required for access to this command.

Note: It is possible for both the “:” and the “+” commands to be active at the same time. The “+” command determines whether the sensor is allowed to transmit data. So if this were the case, the “:” command must also be turned off to allow the free flow of data.

8. An “*” command will suppress or restore the initialization message in the Decimal ASCII mode. This command will toggle the transmitting of the text header during initialization (On to Off; Off to On). This change is made non-volatile in the unit on EEPROM by keying in the quote (“) character. Command mode is required for access to this command.
9. An “&” command brings up a menu which allows any of several parameters to be set. These are system time constants, selection of data channels for serial output, and baud rates. This change is made non-volatile in the unit on EEPROM by keying in the quote (“) character. Command mode is required for access to this command.

The commands “~”, “@”, “#”, “\$”, “(”, “)”, “{”, “}”, “|”, “<”, “>” and “?” are used by the Watson factory to calibrate the unit and should be used only with the assistance of the factory. If an undesired function is called, a “Q”, and sometimes Escape or a Delete will interrupt the command and return to operation with the least disturbance to the system. All other unspecified characters such as carriage return, line feed and space are ignored by the system.

If there are problems with the system “hanging up” during the binary output mode, check for crosstalk between the serial transmit and receive line in your installation. In addition, check to see that the communications program used is not sending an echo. This will not happen in the decimal or hexadecimal modes because command characters recognized by the system are not produced in those modes.

Analog Outputs

Analog signal is output from a 14 bit digital to analog converter through an operational amplifier. Each analog output has a 300 ohm resistor in series to eliminate oscillations from high capacitance loads. The output range for the analog output channels are user selectable between unipolar (0-5 VDC) or bipolar (± 5 VDC). See Appendix B for information on selecting unipolar or bipolar output. The analog outputs are referenced to the common signal ground Pin 8. The analog outputs can be found on the 12-pin connector. The outputs include:

<u>Signal</u>	<u>Pin</u>	<u>Range</u>	<u>Bipolar Output (± 5VDC)</u>		<u>Unipolar Output (0 to 5 VDC)</u>	
			<u>Zero Rate ($0^\circ/s$)</u>	<u>Scale Factor</u>	<u>Zero Rate ($0^\circ/s$)</u>	<u>Scale Factor</u>
Angular Rate 1	10	$\pm 400^\circ/s$	0 VDC	$80^\circ/s/V$	2.5 VDC	$160^\circ/s/V$
Angular Rate 2	3	$\pm 200^\circ/s$	0 VDC	$40^\circ/s/V$	2.5 VDC	$80^\circ/s/V$
Angular Rate 3	9	$\pm 100^\circ/s$	0 VDC	$20^\circ/s/V$	2.5 VDC	$40^\circ/s/V$
Angular Rate 4	2	$\pm 50^\circ/s$	0 VDC	$10^\circ/s/V$	2.5 VDC	$20^\circ/s/V$

Built in Test Digital Output

Built-In Test is an active low digital output that continuously monitors the internal sensors for faults. This signal is available on pin 5 of the connector. This output is High (5VDC) when the unit is operating normally. This output is Low (ground) when a fault is indicated. Flag reset is normal operation. The fault condition is set if the Angular Rate sensor has failed or the sensors temperature range has been extended.

Specifications

Angular Rate

Ranges:	$\pm 50^\circ/\text{sec}$	$\pm 100^\circ/\text{sec}$	$\pm 200^\circ/\text{sec}$	$\pm 400^\circ/\text{sec}$
Resolution:	$0.006^\circ/\text{sec}$	$0.012^\circ/\text{sec}$	$0.024^\circ/\text{sec}$	$0.05^\circ/\text{sec}$
Analog Scale Factor:	Bipolar Unipolar	$100\text{mV}/^\circ/\text{sec}$ $50\text{mV}/^\circ/\text{sec}$	$50\text{mV}/^\circ/\text{sec}$ $25\text{mV}/^\circ/\text{sec}$	$25\text{mV}/^\circ/\text{sec}$ $12.5\text{mV}/^\circ/\text{sec}$ $6.25\text{mV}/^\circ/\text{sec}$
Scale Factor Accuracy:	0.2%			At constant room temperature
Scale Factor Temp Coefficient:	0.1%			Over temperature range
Bias:	$\pm 0.1^\circ/\text{sec}$			At room temp
Bias: Over Temp Range	$\pm 0.2^\circ/\text{sec}$			
Warmup Drift:	$\pm 0.25^\circ/\text{sec}$			
Non-Linearity:	$< 0.15\%$			Full scale range
Bandwidth:	70 Hz (Typical)			User selectable 5 to 200 Hz
Noise:	$< 0.05^\circ/\text{sec rms}$			1 Hz to 100 Hz

Environmental

Temperature: Operating	-40°C to $+85^\circ\text{C}$		
Temperature: Storage	-55°C to $+85^\circ\text{C}$		
Vibration: Operating	5g rms		20 Hz to 2 KHz
Vibration: Survival	10g rms		20 Hz to 2 KHz
Shock: Survival	500g		10mS 1/2 sine wave

Electrical


Frame Rate:	800 Hz		Maximum
Startup Time: Data	5 sec		
Startup Time: Fully operational	10 sec		
Input Power:	8 to 45VDC		0.7W
Input Current:	45mA @ 12VDC		20mA @ 24VDC
Digital Output:	RS-232		± 399.99 Range
Analog Output:	User Selectable		$\pm 5\text{VDC}$ Bipolar ; $0-5\text{VDC}$ Unipolar
Analog Output Impedance:	300 Ohm		Per line

Physical

Size: Including Mounting Flanges	1.2"W x 2.8"L x 1.35"H		3.0 x 7.1 x 3.0 (cm)
Weight:	2.1 oz		60 grams
Connection:	Amp 4-794627-2 (12 pin)		

- Specifications are subject to change without notice.
- This product may be subject to export restrictions. Export Classification ECCN 7A994

Connections

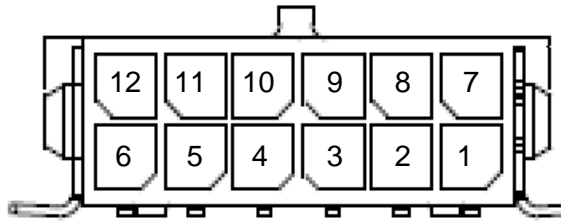

Pin	Description
1	RS-232 TXD
2	Angular Rate Analog Output 4 ($\pm 50^\circ/\text{sec}$ range)
3	Angular Rate Analog Output 2 ($\pm 200^\circ/\text{sec}$ range)
4	No Connection
5	Built in Test (BIT) Output
6	Power Ground
7	RS-232 RXD
8	Signal Ground
9	Angular Rate Analog Output 3 ($\pm 100^\circ/\text{sec}$ range)
10	Angular Rate Analog Output 1 ($\pm 400^\circ/\text{sec}$ range)
11	Factory use (Do not Connect)
12	+Vin Power +8 to +45 VDC

The RS-232 serial and analog output connections are referenced to Signal Ground on pin 8. The power ground is already connected internally to the signal ground.

Dimensions

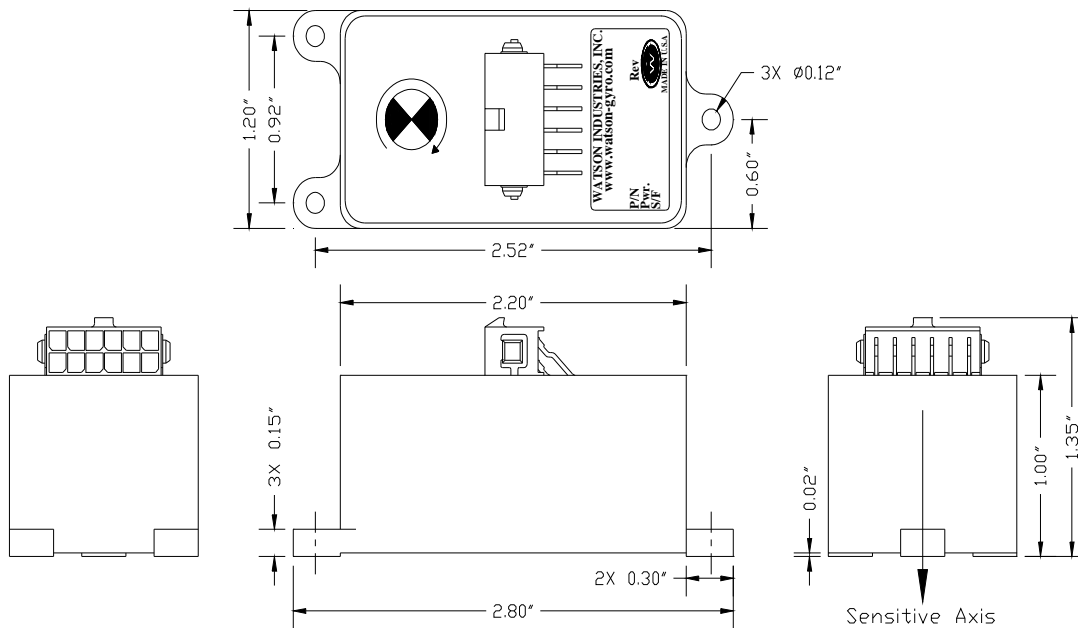


Figure 2

WARNING

Rough handling or dropping of this unit is likely to cause damage. Over-voltage and/or miswiring of this unit will cause damage. This unit should be protected against prolonged exposure to high humidity and/or salt air environments.

DISCLAIMER

The information contained in this manual is believed to be accurate and reliable; however, it is the user's responsibility to test and to determine whether a Watson Industries' product is suitable for a particular use.

Suggestion of uses should not be taken as inducements to infringe upon any patents.

WARRANTY

Watson Industries, Inc. warrants, to the original purchaser, this product to be free from defective material or workmanship for a period of two full years from the date of purchase. Watson Industries' liability under this warranty is limited to repairing or replacing, at Watson Industries' sole discretion, the defective product when returned to the factory, shipping charges prepaid, within one full year from the date of purchase. The warranty described in this paragraph shall be in lieu of any other warranty, express or implied, including but not limited to any implied warranty of merchantability or fitness for a particular purpose.

Excluded from any warranty given by Watson Industries are products that have been subject to abuse, misuse, damage or accident; that have been connected, installed or adjusted contrary to the instructions furnished by seller; or that have been repaired by persons not authorized by Watson Industries.

Watson Industries reserves the right to discontinue models, to change specifications, price or design of this product at any time without notice and without incurring any obligation whatsoever.

The purchaser agrees to assume all liabilities for any damages and/or bodily injury that may result from the use, or misuse, of this product by the purchaser, his employees or agents. The purchaser further agrees that seller shall not be liable in any way for consequential damages resulting from the use of this product.

No agent or representative of Watson Industries is authorized to assume, and Watson Industries will not be bound by any other obligation or representation made in connection with the sale and/or purchase of this product.

PRODUCT LIFE

The maximum expected life of this product is 20 years from the date of purchase. Watson Industries, Inc. recommends the replacement of any product that has exceeded the product life expectation.

Customer Service

All repairs, calibrations and upgrades are performed at the factory. Before returning any product, please contact Watson Industries to obtain a Returned Material Authorization number (RMA).

Return Address & Contact Information

Watson Industries, Inc.
3035 Melby Street
Eau Claire, WI 54703
ATTN: Service Department
Telephone: (715) 839-0628 Fax: (715) 839-8248 email: support@watson-gyro.com

Returning the Product

Product shall be packaged making sure there is adequate packing around all sides. Correspondence shall include:

- Customer's Name and Address
- Contact Information
- Equipment Model Number
- Equipment Serial Number
- Description of Fault

It is the customer's responsibility to pay all shipping charges from customer to Watson Industries, including import and transportation charges.

Appendix A

The following outputs are available via the RS-232 serial link. Their full-scale ranges are listed for both decimal and binary format.

<u>Inertial Output</u>	<u>Label</u>	<u>Full Scale Decimal</u>	<u>Full Scale Binary</u>
Time Since Reset	TM	65535	16383
Angular Rate	XR	± 399.99 °/s	± 400 °/s
Temperature	TP	-40° to 88°C	-40° to 88°C (7 bit)
Flag Bits	FL	3 ASCII chars representing Octal digits	1 byte
Status Bits	ST	3 ASCII chars representing Octal digits	1 byte
Built In Test (BIT) Status Bits	BT	3 ASCII chars representing Octal digits	1 byte

The Flag Bits contain the following information:

Bit	Description (If Set)
0	Unused
1	Unused
2	Unit Temp Out of Range Flag
3	BIT Test Flag
4	Angular Rate Out of Range Flag
5	Unused
6	Checksum Error Flag
7	Unused

Example: The Flag channel output in ASCII Decimal is "020"

Octal Digit	0		2			0		
Binary Equivalent	0	0	0	1	0	0	0	0
Flag Bit #	7	6	5	4	3	2	1	0

This translates into the information below:

Bit 7	Reset	
Bit 6	Reset	No Checksum Error
Bit 5	Reset	
Bit 4	Set	Angular Rate Out Range (>400 °/s)
Bit 3	Reset	No BIT Error
Bit 2	Reset	Unit Temp in Range (-40° to +85° C)
Bit 1	Reset	
Bit 0	Reset	

The Status Bits contain the following information:

Bit	Description
0	Unused
1	Unused
2	Unused
3	Unused
4	If set, Unit is in Initialization
5	Unused
6	If set, Command Mode is Selected
7	Unused

Example: The Status channel output in ASCII Decimal is "120"

Octal Digit	1		2			0		
Binary Equivalent	0	1	0	1	0	0	0	0
Status Bit #	7	6	5	4	3	2	1	0

This translates into the information below:

Bit 7 Reset
 Bit 6 Set Command mode active
 Bit 5 Reset
 Bit 4 Set In Initialization
 Bit 3 Reset
 Bit 2 Reset
 Bit 1 Reset
 Bit 0 Reset

The Built In Test (BIT) Status Bits contain the following information:

Bit Description
 0 Unused
 1 Unused
 2 Unused
 3 If set, Sensor Temperature out of range
 4 If set, Angular Rate Sensor Failure
 5 Unused
 6 Unused
 7 Unused

Example: The BIT Test channel output in ASCII Decimal is "020"

Octal Digit	0		2			0		
Binary Equivalent	0	0	0	1	0	0	0	0
BIT Status Bit #	7	6	5	4	3	2	1	0

This translates into the information below:

Bit 7 Reset
 Bit 6 Reset
 Bit 5 Set
 Bit 4 Set Rate Sensor Failure
 Bit 3 Reset Temp Sensor in range
 Bit 2 Reset
 Bit 1 Reset
 Bit 0 Reset

Appendix B

Activating Command Mode (Double Spacebar Mode)

- 1) Connect the unit to a DC power source that is off.
- 2) The viewing computer needs a valid bi-directional RS-232 serial port. Connect the serial port of the Watson sensor to the computer's serial port.
- 3) Open a terminal program (such as HyperTerminal) to interface with the unit. The default baud rate of the unit is 9600 baud. Make sure the computer's serial port is open.
- 4) Power-on the unit. A startup message will be transmitted by the unit and will appear in the terminal window unless it has been suppressed (See RS-232 Input Commands above).
- 5) During initialization, hit the space bar twice within close succession.

Note: The sensor initialization time begins after the startup message is transmitted. Typically, this time period lasts 5 seconds, but could be as long as 127 seconds depending on your sensor.

- 6) Wait until after initialization is finished. At this point, command mode will be activated and the unit will accept keyboard commands.

Note: Most Watson sensors have initialization times that are shorter than 30 seconds. Any extra keystrokes (other than two spacebars) sent during initialization will deactivate command mode.

**It can often take a few attempts to get the hang of step 5. Repeat steps 4-6 until successful.

Accessing the Main Menu

- 1) Activate Command Mode (See above)
- 2) Typing '&' will bring up the main menu:

```
TYPE IN THE NUMBER OF YOUR SELECTION (OR 'Q' TO QUIT):  
  1 = SET OUTPUT CHANNELS  
  2 = LIST CURRENT OUTPUT CHANNEL SELECTION  
  3 = SET ANALOG VOLTAGE RANGE  
  4 = SET OUTPUT BANDWIDTH  
  5 = SET BINARY OUTPUT FORMAT  
  6 = SET NEW BAUD RATE
```

Appendix B.1 Set Output Channels

- 1) To change the output channels, type '1' at the main menu.
This will bring up the following message:

```
TO SET FOR OUTPUT FOR ANY OF THE FOLLOWING DATA ITEMS, PRESS Y  
TO AVOID ANY OF THE FOLLOWING DATA ITEMS, PRESS N  
TO QUIT AND DISREGARD ANY OTHER DATA, PRESS Q  
  
*** DO YOU WANT TO PROCEED? (Y/N/Q)
```

- 2) To proceed type 'Y'. Stop this process by typing either 'N' or 'Q'.
If 'Y' is pressed, each channel will come up one at a time.
For example:

```
DO YOU WANT OUTPUT TIME SINCE RESET?
```

- 3) Type 'Y' to output the channel, type 'N' to remove the channel.
After the last channel is listed, this message will appear:

```
Y = GOBACK, N = INSTALL DATA & QUIT, Q = QUIT  
DO YOU WANT TO TRY TO SET DATA AGAIN?
```

- 4) To accept the new channels type 'N'. Typing a 'Y' will start the command sequence over.
Typing a 'Q' at any time in the sequence will quit without updating the channels.

Changes made will not change the non-volatile settings. To make these new settings the default value, send a Quotation Mark (").

- 5) Press the space bar after quitting or updating the new channels to restart the data flow.

Appendix B.2 List Output Channels

- 1) To list the current output channel selection, type '2' at the main menu.
- 2) The sensor will show which channels are currently active.

Appendix B.3 Set Analog Voltage Range

- 1) To update the analog output voltage range, type '3' at the main menu.
This will bring up the menu:

```
THE CURRENT SETTING IS: BIPOLAR  
  
SELECT ANALOG VOLTAGE RANGE (OR 'Q' TO QUIT):  
1 = UNIPOLAR 0 TO 5 VDC RANGE (0 DEG/SEC = 2.5VDC)  
2 = BIPOLAR +/-5 VDC RANGE (0 DEG/SEC = 0.0VDC)
```

- 2) To change the analog voltage range to Unipolar, type '1' at this menu.
To change the analog voltage range to Bipolar, type '2' at this menu.
- 3) Changes made will not change the non-volatile settings. To make these new settings the default value, send a Quotation Mark (").
- 4) Press the space bar after quitting or updating the output range to restart the data flow.

Appendix B.4 Set Output Bandwidth

To change the bandwidth for the angular rate output, type '4' at the main menu.
This will bring up the menu:

```
THE CURRENT SETTING IS: 070 Hz
TYPE IN NEW BANDWIDTH IN Hz (OR 'Q' TO QUIT):
  (UP TO 3 DIGITS - RANGE 5 TO 200):
```

- 1) To change type in the new bandwidth in Hz, followed by an <Enter> if typing in less than 3 digits.
(e.g. to change to 50 Hz type in '50' followed by <Enter> or '050')
(e.g. to change to 5 Hz type in '5' followed by <Enter> or '05' followed by <Enter> or '005')
(e.g. to change to 100 Hz type in '100')
- 2) Changes made will not change the non-volatile settings. To make these new settings the default value, send a Quotation Mark (").
- 3) Press the space bar after quitting or updating the binary format to restart the data flow.

Note: If the value entered is outside the acceptable 5 to 200 Hz range then the following message will be displayed.

```
* * * ERROR * * *

THE CURRENT SETTING IS: 070 Hz
TYPE IN NEW BANDWIDTH IN Hz (OR 'Q' TO QUIT):
  (UP TO 3 DIGITS - RANGE 5 TO 200):
```

Repeat Step 1.

Appendix B.5 Set Binary Output Format

- 1) To update the binary output format, type '5' at the main menu.

This will bring up the menu:

```
THE CURRENT SETTING IS: 3 BYTE

SELECT BINARY OUTPUT FORMAT (OR 'Q' TO QUIT):
  1 = THREE BYTE BINARY OUTPUT FORMAT
  2 = TWO BYTE BINARY OUTPUT FORMAT
```

- 2) To change the binary output format to three byte, type '1'.
To change the binary output format to two byte, type '2'.

See Appendix C for more information binary formatting.

- 3) Changes made will not change the non-volatile settings. To make these new settings the default value, send a Quotation Mark (“).
- 4) Press the space bar after quitting or updating the binary format to restart the data flow.

Appendix B.6 Set Baud Rate

- 1) To change the baud rate at which the sensor communicates, type ‘6’ at the main menu. This will bring up the menu:

```
TYPE IN THE NUMBER OF YOUR SELECTION (OR 'Q' TO QUIT):  
(EFFECTIVE IMMEDIATELY - SAVE TO MAKE PERMANENT)  
  1 = 38.4 K BAUD  
  2 = 19.2 K BAUD  
  3 =  9.6 K BAUD  
  4 =  4.8 K BAUD
```

- 2) Change the baud rate to a new setting.

To change to 38,400 Baud, type ‘1’.
To change to 19,200 Baud, type ‘2’.
To change to 9,600 Baud, type ‘3’.
To change to 4,800 Baud, type ‘4’.

The baud rate change will take effect immediately. To make the new baud rate the default setting, send a quote symbol (“) using the new baud rate. Otherwise the old baud rate will return the next time the unit is powered up.

Note: The baud rate of the software that is communicating to the sensor will need to be changed to match the new setting.

- 3) Press the space bar to resume data transmission.

Note: The factory settings for serial communications are 9.6K baud with 8 bits and one stop bit, no parity.

Appendix C Binary Output Format

Appendix C.1 Two Byte Binary Angular Rate Data Format

All of the data words have a high sign bit (bit 7), but the delimiter byte is an ASCII carriage return character that has a low sign bit (bit 7). One word (two bytes) is transmitted per output parameter.


Example: Unit is sending out Angular Rate
The Unit is seeing these conditions:

Angular Rate
-100.24°/s

Binary Output Format:

Word1	<CR> byte
0xEFBB	0x0D

The Carriage return byte is the only byte which has a value less than 128 (0x80). This is the Synchronizing Byte.

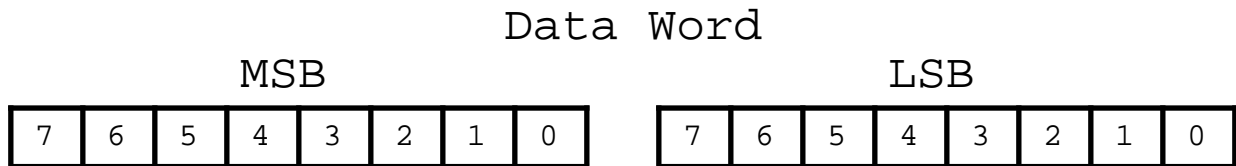

Bit 7 of the MSB is set to 1. Bits 6 to 0 of the MSB are the upper 7 bits of the data. (sign plus 6 bits of data)
Bit 7 of the LSB is set to 1. Bits 6 to 0 of the LSB are the lower 7 bits of the data.

After the two byte data word is received, the LSB is shifted left to shift out the 7th bit (always set to 1). The MSB is then connected to the LSB as a 16-bit word. This word is then shifted left to shift out the 7th bit in the MSB (always set to 1). What remains is a signed fractional word with a resolution of 13 bits plus a sign bit. Scale factor: 0.0122 °/s/bit

To convert binary data:

Angular Rate
0xEFBB

Split each word into two bytes:

Angular Rate
0xEF
0xBB

Remove the most significant bit from each byte:

Angular Rate
0x6F 0x3B

Shift lower byte left once (to remove 1 bit space between bytes):

Angular Rate
0x6F 0x76

Shift lower & upper bytes left once (to remove 1 bit space at top of high byte):

Angular Rate
0xDF 0xEC

Convert from hexadecimal to decimal counts:

Angular Rate
57324

Correct bank, elevation, and angular rates for the sign
If >32767 then subtract 65536 from the data

X Rate
-8212

Multiply the data (in counts) by the scale factor
Convert to units: counts * scale factor
For Angular Rate: Scale factor is: (400 °/s) / 32768 counts

Angular Rate
-100.24 °/s

The nominal interface settings are:

9600 Baud
8 Bit Data
1 Start Bit
1 Stop Bit
No Parity

Appendix C.2 Three Byte Binary Angular Rate Data Format

All of the data words have a high sign bit (bit 7), but the delimiter byte is an ASCII carriage return character that has a low sign bit (bit 7). Three bytes are transmitted per output parameter.

Example: Unit is sending out Angular Rate
The Unit is seeing these conditions:

Angular Rate
100.23°/s

Binary Output Format:

Byte 1	Byte 2	Byte 3	<CR> byte
0x90	0x84	0xDB	0x0D

The Carriage return byte is the only byte which has a value less than 128 (0x80). This is the Synchronizing Byte.

3 Byte Binary Angular Rate Data Format																							
7	6	5	4	3	2	1	0	7	6	5	4	3	2	1	0	7	6	5	4	3	2	1	0
High Byte								Middle Byte								Low Byte							

Bit 7 of the High Byte is set to 1. Bits 6 to 0 of the High Byte are the upper 7 bits of the data. (sign plus 6 bits of data)

Bit 7 of the Middle Byte is set to 1. Bits 6 to 0 of the Middle Byte are the next 7 bits of the data.

Bit 7 of the Low Byte is set to 1. Bits 6 to 0 of the Low Byte are last 7 bits of the data.

After the 3 byte data word is received, the Low Byte is shifted left to shift out the 7th bit(always set to 1). The Middle Byte is then connected to the Low Byte as a 16 bit word. This 16 bit word is then shifted left to shift out the 7th bit in the Middle Byte (always set to 1). The High Byte is then connected to the 16 bit word to form a 24 bit "word". This 24 bit "word" is then shifted left to shift out the 7th bit in the High Byte (always set to 1). What remains is a signed fractional 3 byte answer with a resolution of 20 bits plus a sign bit. Scale factor: 0.000381 °/s /bit

$$0x7FFFF8 = +399.999 \text{ °/s}$$

$$0x7FFFF0 = +399.996 \text{ °/s}$$

...

$$0x000008 = +0.0004 \text{ °/s}$$

$$0x000000 = +0.0000 \text{ °/s}$$

$$0xFFFFF8 = -0.0004 \text{ °/s}$$

...

$$0x800008 = -399.996 \text{ °/s}$$

$$0x800000 = -400.000 \text{ °/s}$$

To convert binary data:

Angular Rate		
Byte 1	Byte 2	Byte 3
0x90	0x84	0xDB

Shift Byte 3 left once to remove the high bit (bit 7) of the low byte:

Angular Rate		
Byte 1	Byte 2	Byte 3
0x90	0x84	0xB6

Shift lower Word (Byte2:Byte3) left once to remove the high bit (bit 7) of the middle byte:

Angular Rate		
Byte 1	Byte 2	Byte 3
0x90	0x09	0x6C

Shift all 3 bytes left once to remove the high bit (bit 7) of the high byte:

Angular Rate		
Byte 1	Byte 2	Byte 3
0x20	0x12	0xD8

Convert from hexadecimal to decimal counts:

Angular Rate
2101976

Correct angular rate for the sign

If >8388607 then subtract 16777216 from the data

Angular Rate
2101976

Multiply the data (in counts) by the scale factor

Convert to units: counts * scale factor

For Angular Rate: Scale factor is: (400 °/s) / 8388608 counts

Angular Rate
100.23 °/s

The nominal interface settings are:

9600 Baud
8 Bit Data
1 Start Bit
1 Stop Bit
No Parity